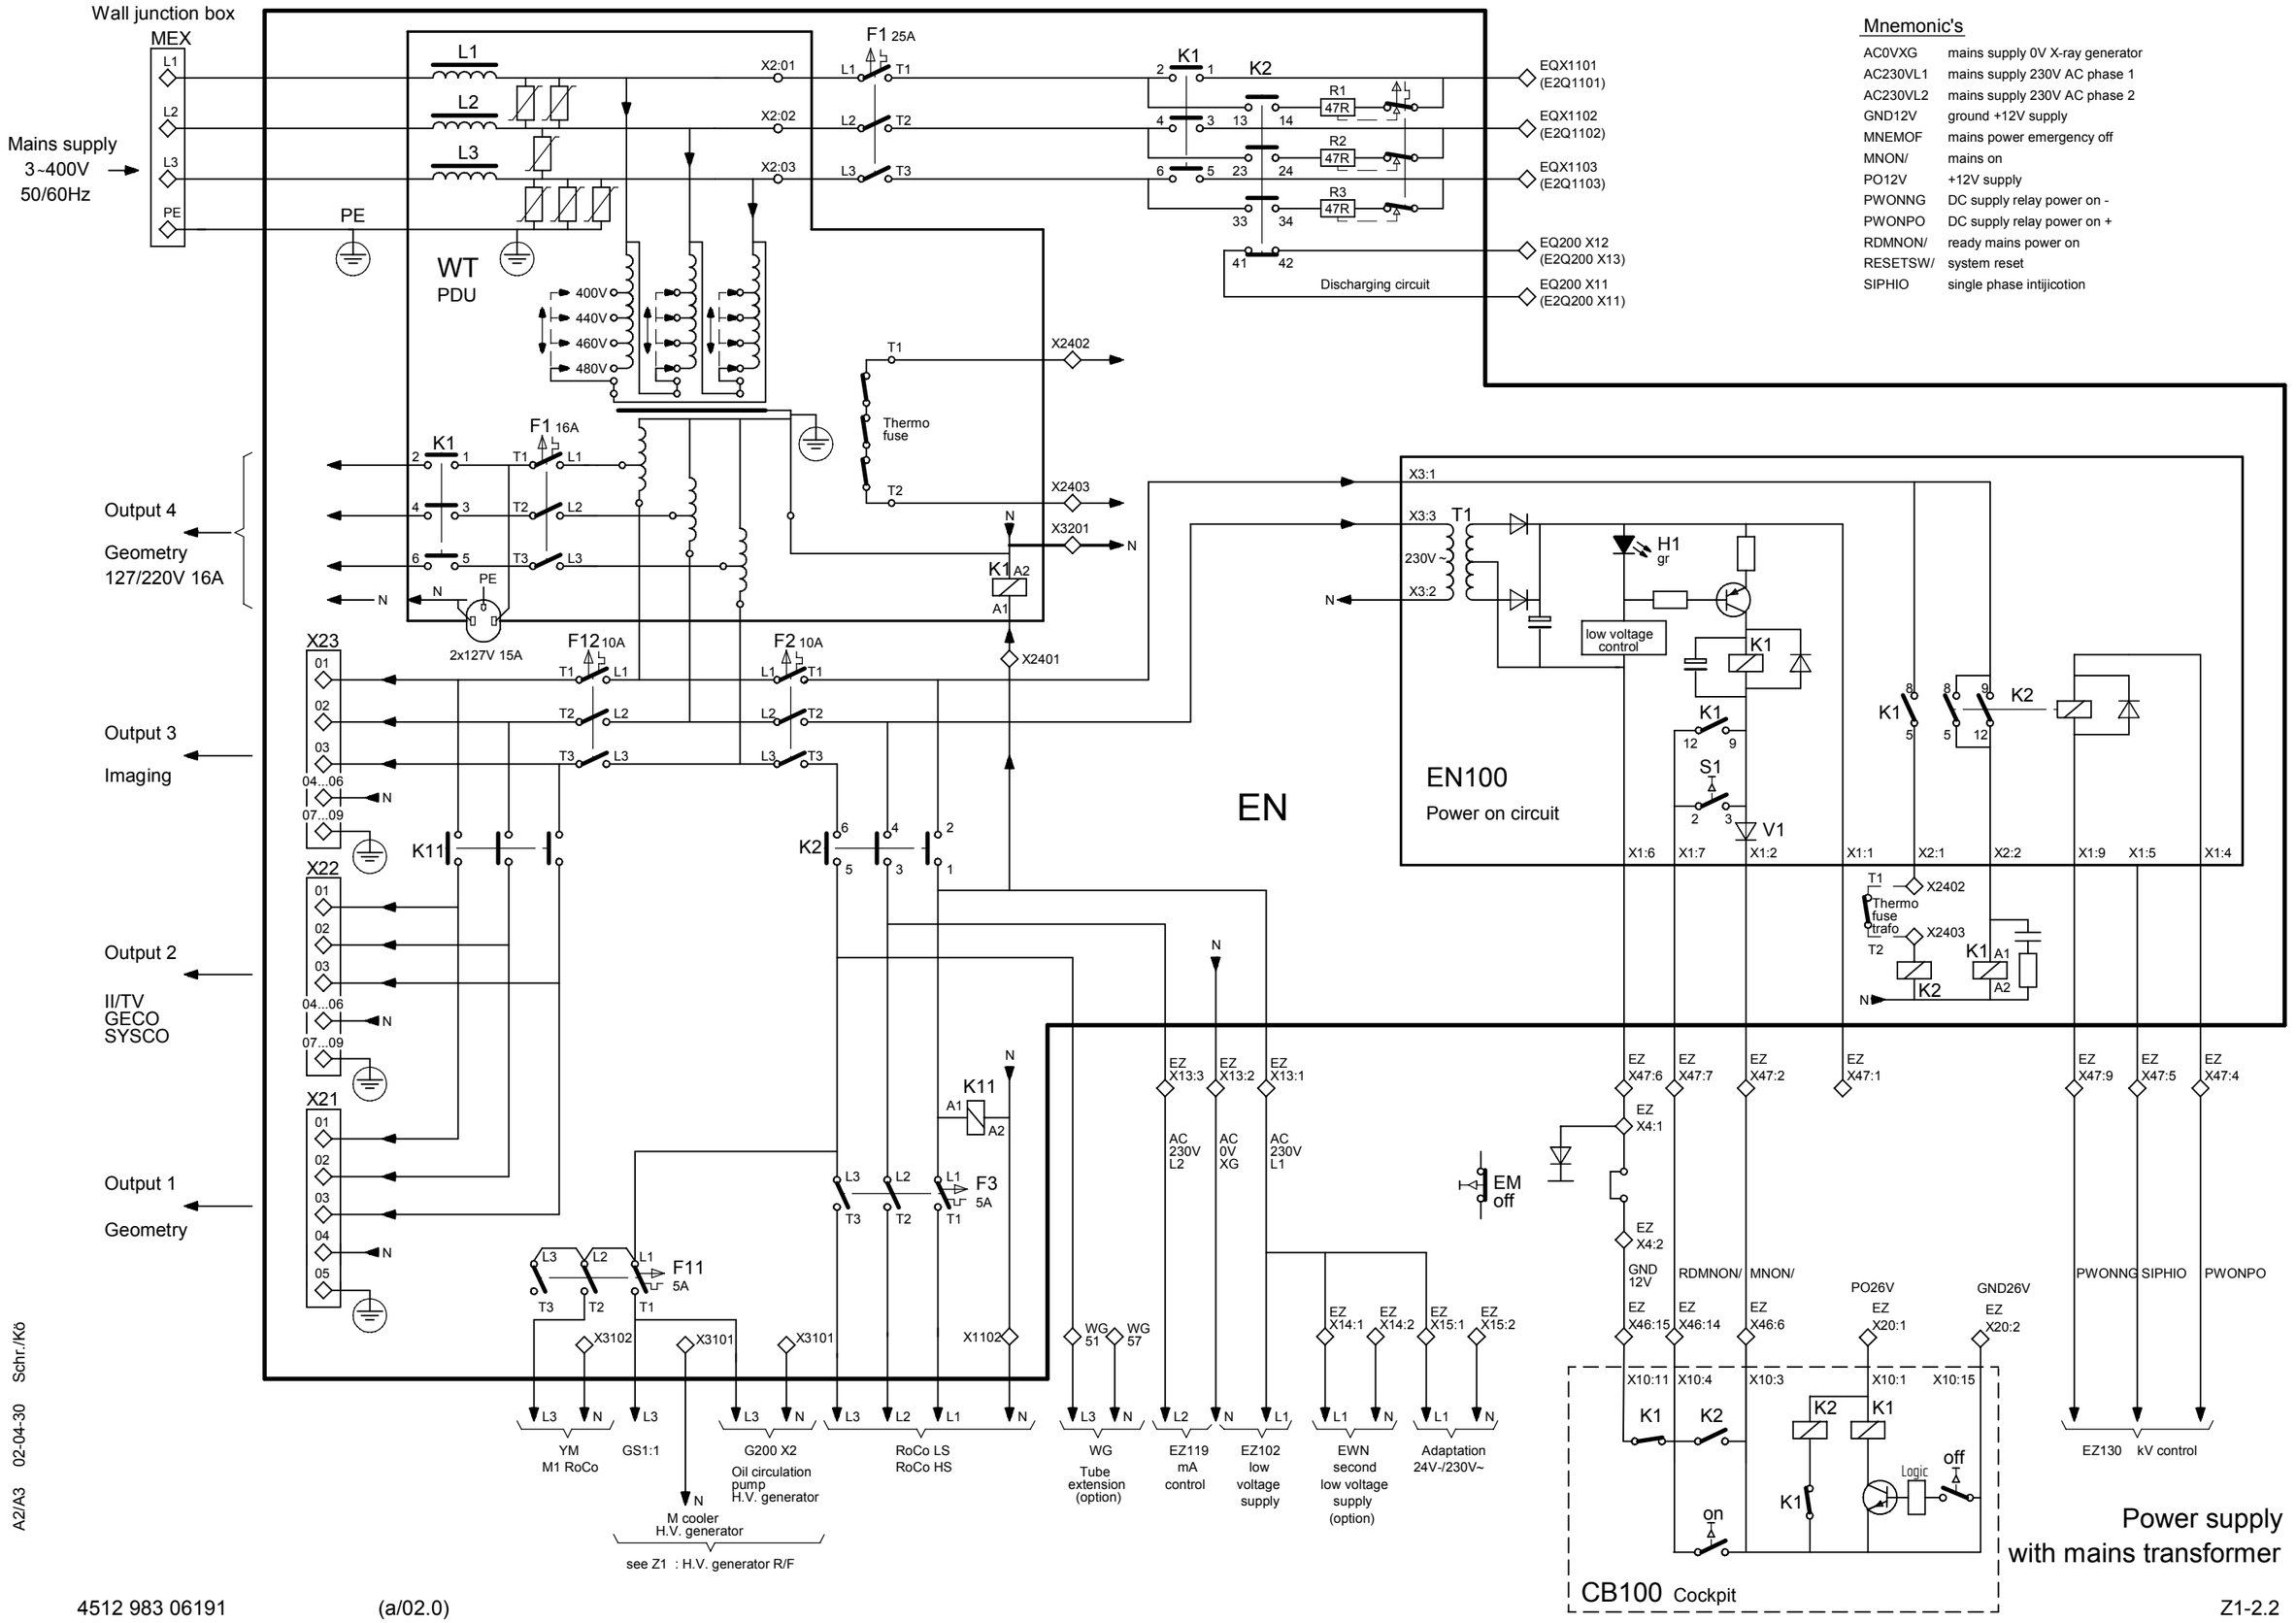

Mnemonic's

AC0VXG	mains supply 0V X-ray generator
AC230VL1	mains supply 230V AC phase 1
AC230VL2	mains supply 230V AC phase 2
GND12V	ground +12V supply
MNEMOF	mains power emergency off
MNON/	mains on
PO12V	+12V supply
PWONNG	DC supply relay power on -
PWONPO	DC supply relay power on +
RDMNON/	ready mains power on
RESETSW/	system reset
SIPHIO	single phase intjicotion

A2/A3 02-04-30 Schr./Kö

4512 983 06191 (a/02.0)

© Philips Medical Systems